

# Medtronic

## IN.PACT™ 018

Drug-Coated Balloon (DCB)†

0.018" DCB  
platform

# Low profile. High performance.<sup>1</sup>

Choose the low-profile DCB with trusted technology  
and designed for better deliverability.†



Crosses tight lesions

## 5 F

5 Fr compatible  
(4-6 mm diameter)



Available in 80 and  
130 cm catheter lengths



Same drug formulation of  
IN.PACT Admiral™ DCB§

†Data on file with Medtronic.

‡Licenced as IN.PACT 018 Paclitaxel-Coated PTA Balloon Catheter.

§Licenced as IN.PACT Admiral Paclitaxel-Coated PTA Balloon Catheter.

# Expand your treatment options for femoropopliteal disease with the IN.PACT 018 drug-coated balloon (DCB)

## Low-profile design

The IN.PACT 018 DCB features a low-profile design engineered to:

Provide improved deliverability†

Work with 0.018" guidewires

Allow the option to treat via femoral access with 80 and 130 cm catheter lengths


## Peel-away balloon protector

The IN.PACT 018 DCB features a peel-away balloon protector that helps preserve the integrity of the drug coating.


†Data on file with Medtronic.

## Building on proven<sup>3</sup> technology


The IN.PACT 018 DCB brings the proven<sup>3</sup> drug formulation of the IN.PACT Admiral DCB to a new platform, so interventionalists can expect the same sustained efficacy and safety.

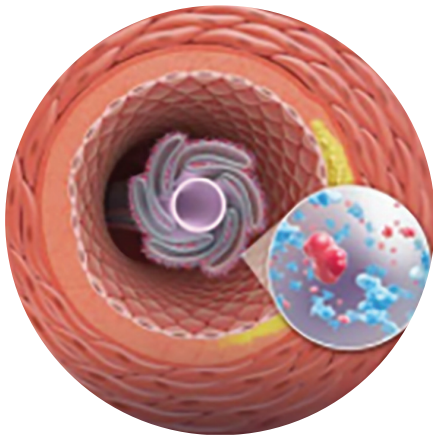

Efficient drug transfer

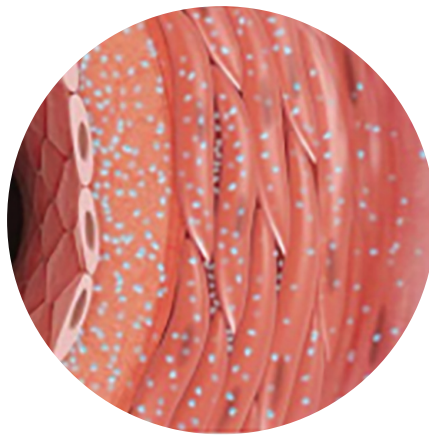

180 days of drug in tissue<sup>1</sup>

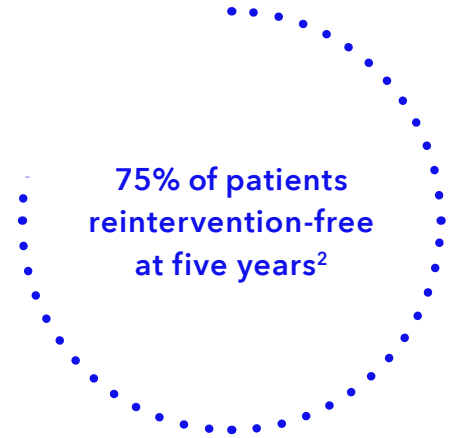

Extended effect

## Expanded platform, trusted data

Medtronic IN.PACT 018 and IN.PACT Admiral drug-coated balloons allow you to:

- Choose your preferred treatment algorithm
- Minimize guidewire exchanges
- Deliver long-term clinical outcomes<sup>2</sup>

**Highest**

patency benefit  
through three years<sup>2</sup>

**Lowest**

CD-TLR rates  
through five years<sup>2</sup>

**Most**

publications  
for a DCB<sup>§</sup>

The safety and effectiveness of the IN.PACT Admiral DCB (.035 in guidewire compatible), as established in the clinical studies that were performed primarily via femoral access, can be considered supportive for the IN.PACT 018 DCB. The IN.PACT 018 DCB has not been evaluated in a clinical study.

<sup>§</sup>List of publications on file with Medtronic.

# Ordering information

IN.PACT 018 Drug-Coated Balloon

130 cm catheter length

Size matrix		40 mm	60 mm	80 mm	100 mm	120 mm	150 mm
5 F	4 mm	IPU04004013P	IPU04006013P	IPU04008013P	IPU04010013P	IPU04012013P	IPU04015013P
	5 mm	IPU05004013P	IPU05006013P	IPU05008013P	IPU05010013P	IPU05012013P	IPU05015013P
	6 mm	IPU06004013P	IPU06006013P	IPU06008013P	IPU06010013P	IPU06012013P	IPU06015013P
6 F	7 mm	IPU07004013P	IPU07006013P	IPU07008013P			

To place an order, contact your Medtronic field representative.

### References

- <sup>1</sup> PMA P140010: Summary of safety and effectiveness data. U.S. Food & Drug Administration. Available at: <https://www.accessdata.fda.gov/scripts/cdrh/cfdocs/cfpma/pma.cfm?id=p140010>. Accessed May 3, 2022.
- <sup>2</sup> Laird JA, Schneider PA, Jaff MR, et al. Long-Term Clinical Effectiveness of a Drug-Coated Balloon for the Treatment of Femoropopliteal Lesions. 5-year results from the IN.PACT SFA Trial. *Circ Cardiovasc Interv.* June 2019;12(6):e007702.
- <sup>3</sup> Data on file with Medtronic. Report numbers: 10191378DOC, 10644925DOC, D00261893.

For a listing of indications, contraindications, precautions, warnings, and potential adverse events, please refer to the Instructions for Use. For applicable products, consult instructions for use on this website <http://manuals.medtronic.com/manuals/main/region>. For any further information, contact your local Medtronic representative.



99 Hereford Street  
Brampton, Ontario, L6Y 0R3  
Toll-free: 800.268.5346  
Tel: 905.460.3800  
[medtronic.ca](http://medtronic.ca)

©2024 Medtronic. All rights reserved. Medtronic, Medtronic logo and Engineering the extraordinary are trademarks of Medtronic. <sup>TM</sup>\*Third party brands are trademarks of their respective owners. All other brands are trademarks of a Medtronic company.  
UC202216387aEC CA-CTL-0365-E Rev. 06/2024